

## Update procedure to the latest version firmware

### [Precautions on updating firmware]

- Please update according to the procedure. Updating with incorrect procedure may cause failure or malfunction of the sound level meter.
- Be sure to supply the power from the AC adapter when updating.
- Do not perform the following operations while updating. It may cause failure or malfunction of the sound level meter.
  - Removing and inserting SD card
  - Disconnection of the sound level meter from the power source
  - Switching the sound level meter to power off
- Back up the necessary conditions before updating. The conditions may be initialized due to firmware update.

### <Update procedure>

- 1 Prepare the update file**
- 2 Start up the sound level meter**
- 3 Switch to the update screen**
- 4 Start update processing**
- 5 Confirm completion of update**

-----\*-----\*-----\*-----\*-----\*-----\*-----\*-----\*-----\*-----

### **1 Prepare the update file**

Download the latest version of the firmware from “LA-7000 series User registration page” of Ono Sokki website (\* User registration is required.)

([https://www.onosokki.co.jp/English/hp\\_e/c\\_support/registration/newregistration.htm](https://www.onosokki.co.jp/English/hp_e/c_support/registration/newregistration.htm))

Rename the file name of the update file downloaded to “LA7000Firmware.dat” and save it in the root directory of the SD card included at the time of purchase.





## 2 Start up the sound level meter

- Select the power supply to "AC adapter"
- ↓
- Turn ON the power
- ↓
- Insert the SD card including the update file into the sound level meter.



## 3 Switch to the update screen

- On menu screen, tap **General** > **About/Update** and switch to the About/Update screen.
- ↓
- Tap "UPDATA"
- ↓
- Tap "OK"
- ↓
- Check that the update screen can be started up.

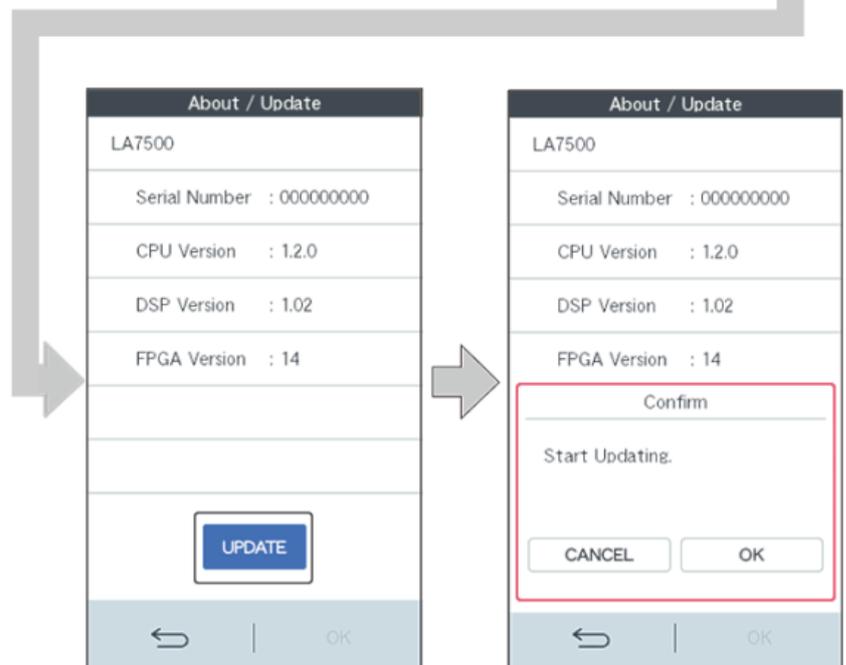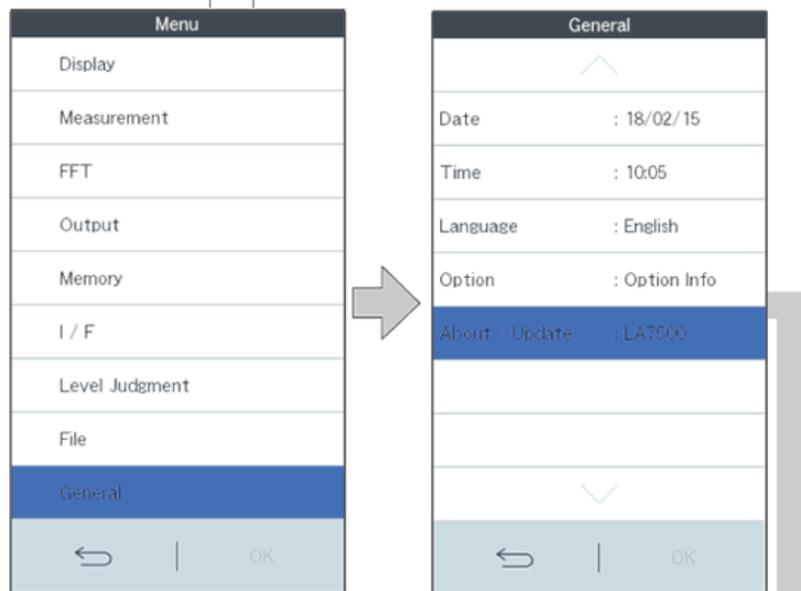

#### 4 Start update processing

Tap **"FIRMWARE UPDATE"** on the update screen.



Confirm that the target version is displayed in the **New Firmware Ver** column.




Tap "Enable" to switch to **"ON"**



Tap **"START UPDATE"**. The screen is switched to the screen showing update processing and update is started.

\*Do not perform the following operations while updating.

- Removing and inserting SD card
- Disconnection of the sound level meter from the power source
- Switching the sound level meter to power OFF

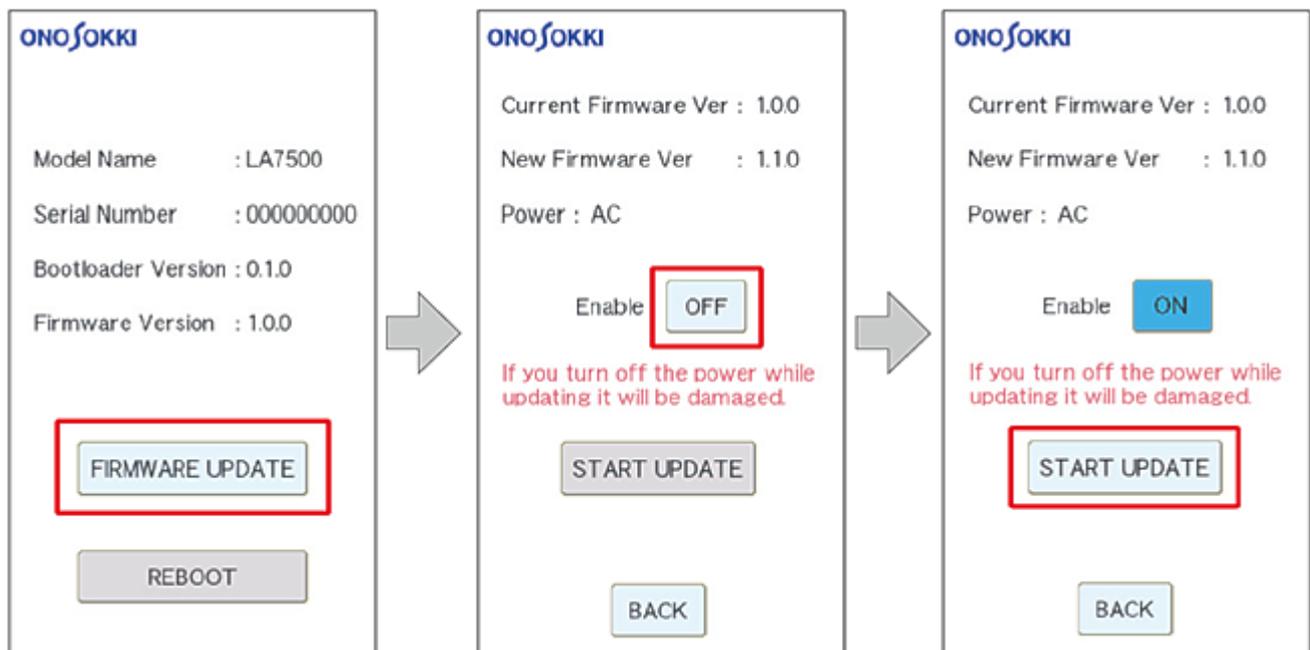

#### 5 Confirm completion of update

Wait until the processing of each item "File Check / Erase / Write / Verify" is completed. (reaching 100%)




Confirm that **"SUCCESS"** is displayed.



Tap **"BACK"** button. The screen returns to the update screen.

- ↓
- Confirm that the version of Firmware Version has been updated
- ↓
- Tap "**REBOOT**" button
- ↓
- The sound level meter automatically restarts and returns to the measurement screen.  
The update is complete.

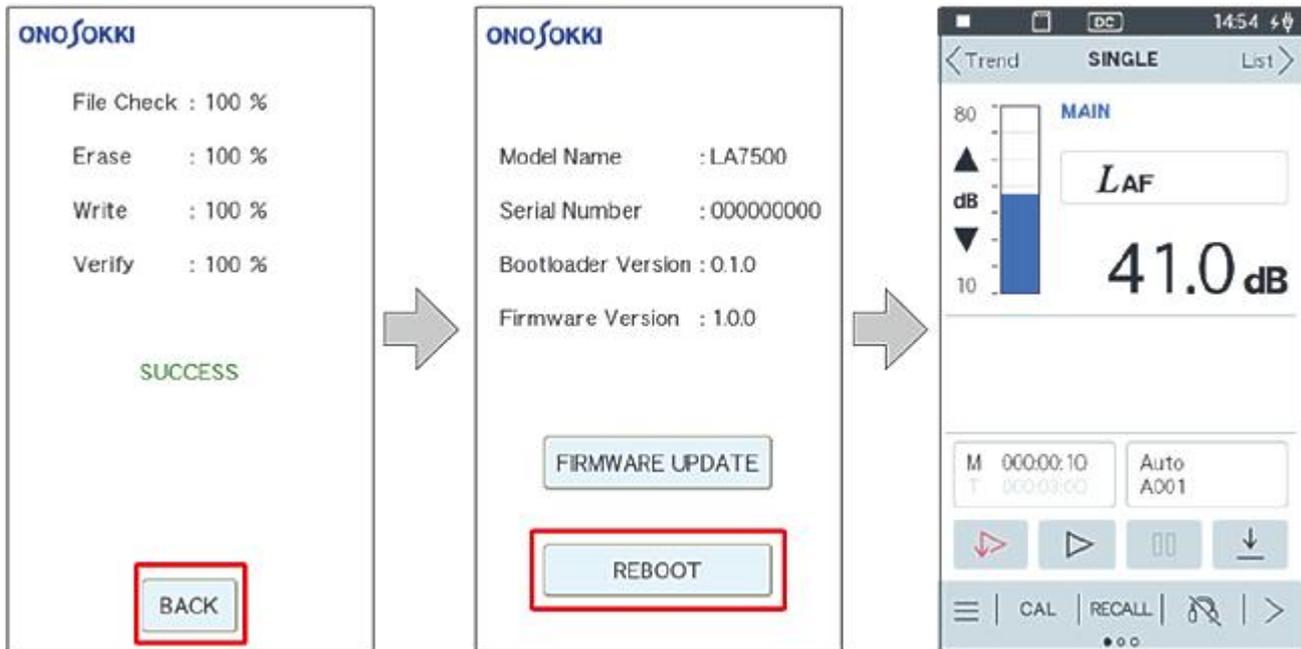

End